#### stryker

# The advanced surgical experience

#### HipMap, HipCheck and Pivot Guardian





# The future of **hip arthroscopy. Now.**

**HipMap, HipCheck, and Pivot Guardian** create an advanced surgical experience for physicians and patients. This is a platform designed to advance FAI through enhanced workflow and improved patient-specific results.

## HipMap

A pre-operative planning tool that delivers a patient-specific, interactive 3D representation of the hip designed to assist with clinical decision making.

#### Plan

HipMap leverages advanced imaging to deliver a report with cam and pincer analysis, version/torsion measurements, indications for potential instability, 3D heat maps, measurement scales, and other visual tools.

HipMap utilizes complex analytics to provide surgeons with an advanced approach to pre-operative clinical decision making.




### Hip**Check**

An intra-operative resection planning and execution tool that allows surgeons to measure and resect cam lesions to a desired alpha angle.

# stryker

#### Educate

HipMap will help patients understand the pathology affecting their hip joint and will contribute to a more robust discussion on the surgical approach.

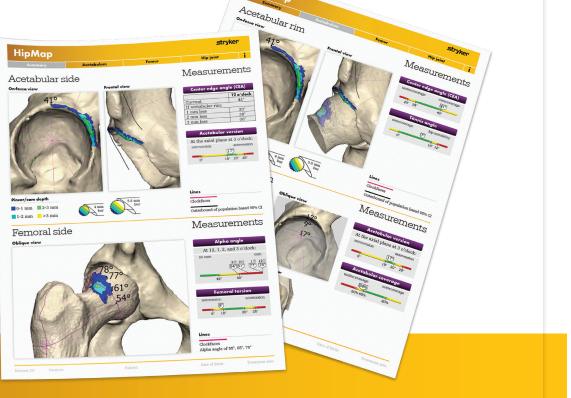

#### Patient-specific cam pathology

Proprietary technology allows surgeons to localize and address cam pathology on a patient-specific basis.

#### Advanced and reproducible approach to femoroplasty

Case review functionality allows surgeons to view a side-by-side comparison of pre-resection and postresection fluoroscopy to verify the resection plan was executed. This checklist provides confidence that the full 3D volume of a cam lesion has been addressed.



#### Improve workflow

Introduces a visualization tool to the sterile field to augment a surgeon's cam resection.

#### **Touchscreen**

The touchscreen interface is designed to integrate into current workflow and put the surgeon in control.

#### **Post-Op communication**

Pre-resection and post-resection comparison images demonstrate the cam was resected appropriately.

# Explore the innovative design

State-of-the-art design and manufacturing focused on improving the patient experience and operating room efficiency.



#### **A.** Traction force gauge

The system includes a traction force gauge that estimates the amount of force on the patient.

#### **B.** Fine and gross traction controls

Designed to provide precise control and better range-of-motion. The surgeon can easily make adduction, abduction, as well as extension and flexion hip adjustments. It also allows for internal and external rotation of the hip.

#### **C.** Post-free

The Pivot Guardian Distraction System is designed to mitigate post related complications.

#### **D.** Carbon fiber construction


Radiolucent carbon fiber construction minimizes the amount of metal components surrounding the hip, allowing for full anterior and posterior visualization during surgery, a "true AP radiographic shot".<sup>1</sup>

#### **OR** turnover

The Pivot Guardian Distraction System is designed to minimize the time and effort required for transport, setup and takedown.

## Discover the next • generation boot

Designed to mitigate heel slip for improved patient outcomes.<sup>2</sup>

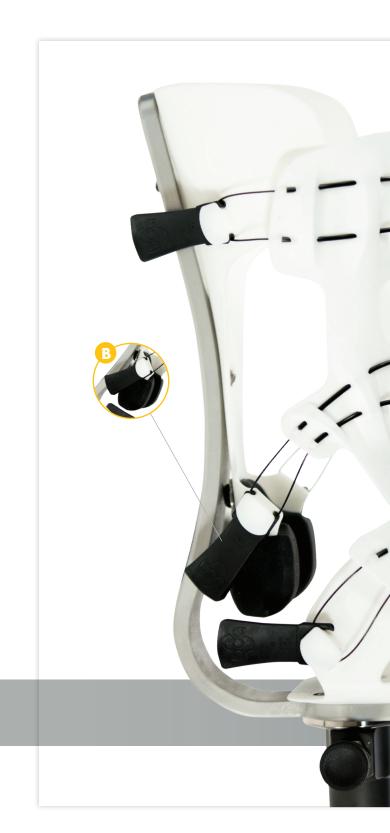




#### A. Boa System

Deliver precise fit and adjustment to distraction system boots, designed to enhance the comfort and safety of the patient.

#### **B.** Achilles block

Designed to secure the patient's ankle during distraction.

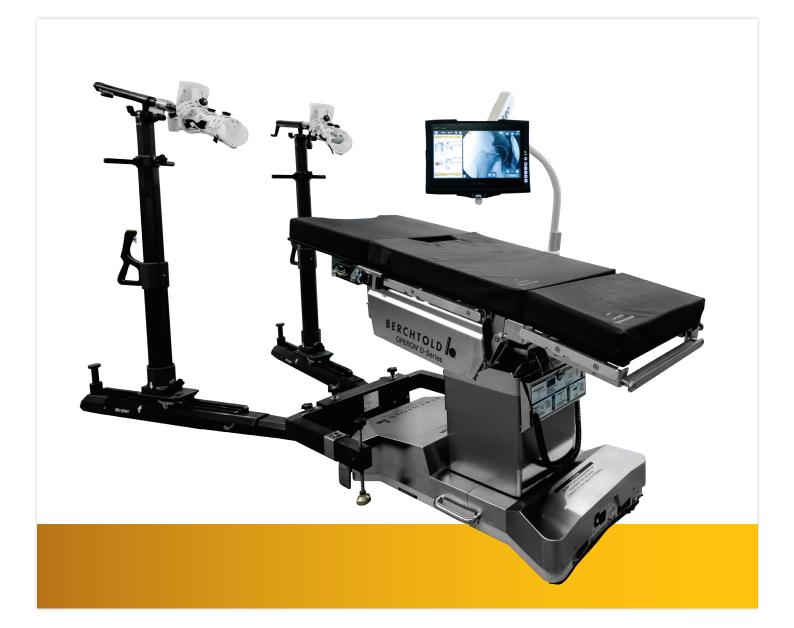

#### **Sports Medicine**

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate a Stryker product. A surgeon must always refer to the package insert, product label and/ or instructions for use, including the instructions for cleaning and sterilization (if applicable), before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its affiliates own, use, or have applied for the following trademarks or service marks: HipCheck, HipMap, Pivot Guardian Distraction System, Stryker. All other trademarks are trademarks of their respective owners or holders.

 Data on file, Stryker, DHD13364, "Hip Distractor, Evaluation of Distracted Space and Imaging"
Data on file, Stryker, DHD13315, "Hip Distractor Competitor Boot Heel Slip, Flame Deflection, and Table Top Pad Shear Detachment Force Benchmarking Report"

Literature Number: 1000903001 Rev A Copyright © 2019 Stryker Stryker Sports Medicine 5670 Greenwood Plaza Blvd, Ste 200 Greenwood Village, CO 80111

www.stryker.com